



TOKRI HIT®





www.tokaihit.com

From the foot of Mt. Fuji to the WORLD



TOKAI HIT Co., Ltd.

306-1, Gendoji-cho, Fujinomiya-shi, Shizuoka-ken, Japan 418-0074 Phone: +81 544 24 6699 FAX: +81 544 24 6641

E-mail: solution@tokaihit.com

It is essential to read the instruction manual when using this device.

- Catalog printed September 2020.
- Specififications and products in the catalog are subject to change without any obligation o the part of the distributor/manufacture.
- Copying and replication of the contents of this images and pictures are strictly prohibited. All Rights Reserved.

for Leica Microsystems



Temp., Humidity and CO2 control instrument for Time-Lapse Imaging

Incubation System for microscopes **Stage Top Incubator**®

Offers precision temperature, humidity and CO2 control for cell culture on a microscope. Enables to conduct short and long term (more than 2 weeks) Time-Lapse Imaging.



Control temperature around a microscope

Enclosure for microscopes ThermoBox

Maintains a stable cell culturing environment.

By enclosing the microscope, it also prevents
the focus drift caused by the thermal expansion of
the microscope itself.



Automatic Thermo-control System (For IVF and basic research)

Glass/Metal Heater for microscopes

ThermoPlate®

Ensures more accurate and reliable thermal control of the specimens during the observation under a microscope. Wide product range supports Biotechnology Science and Industry. 10 year free-repair service for grass breakage* is adopted. *Depending on the models.





Features




Accurate and uniform temperature control

TOKAI HIT Heating Quality

Tokai Hit's original Top Heater is proven to distribute heat uniformly within the Chamber regardless of the type of vessels.





Uniform temperature distribution between wells and within a well


No interference by objective


With unique Top Heater Heating regulation, the bottom of Chamber is access-free for variety of objectives. (No metal plate at the bottom.)



Real-time Sample Feedback Regulation

Sterilized temperature sensor and magnetic lids make it easy to measure the temp. of culture media upon research needs. The controller regulates the heater based on the sensor signal to keep sample at the target temp. accurately.

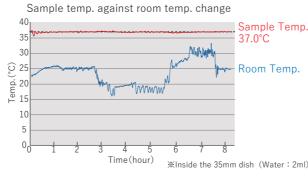



Keeps high-humidity over 95%

Keeps the humidity level inside the chamber more than 95% by heating the distilled water in the Bath Unit. The internal humidifier minimizes the change of concentration of the media by keeping the humidity inside the chamber.





Internal humidifier by Bath Heater

Stable CO₂ environment

The controller mixes 100%CO2 gas and the surrounding air automatically. Stable gas concentration inside the Chamber is kept by sending the mixed gas continuously to the Chamber. (XA case of controller with a built-in digital gas mixer)



Chamber Components

Top Heater --

Main heater which heats the specimen from the upper surface. The transparent glass heater prevents condensation and supports clear visibility.

Dish Fixing Lid -----

Easy setting of vessels with magnetic lid.

Dish Attachment

Supports 35mm dish, 50/60mm dish, chamber slide, slide glass, chambered coverglass and wellplate by changing one-touch mangetic holder.

Bath Unit -----


Keeps distilled water and embedded Bath Heater heats it directly from beneath to generate high-humidity inside the Chamber unit.

- ■ Wreck Proof Lens Heater Cord -:

Easy attachment and detachment with magnet relay connector prevents breakage of objective revolver and lens heater. It is also possible to lock by twisting







■ Easy Dish Fixing -----

for Living cells for your imaging ®

Access Ports

For temperature sensor and tubing for media exchange and drug delivery.


Lens Heater

Prevents heat escaping from the sample to the objective. Especially effective under high magnification, oil/water immersion observation


* Can accommodate objectives up to ϕ 40mm. Thin type and longer type are optional.

Stage Top Incubator Culture Results

| Attribute | Name | Details | Period |
|---------------|--------------------|--|-------------|
| Cultured Cell | STO STO | Embryo; fibroblast, mouse | Over 5 days |
| Cultured Cell | PC12 | Pheochromocytoma; adrenal gland, rat (male) | Over 5 days |
| Cultured Cell | Hela | Adenocarcinoma; crvix, human (female, 31 years) | Over 5 days |
| Primary | Human Embryo | Human embryo in vitro; form fertilization to hatching blastocyst over 7 days | Over 7 days |
| Primary | Neurons | Development of rat cerebral cortical neurons Ove | |
| Primary | Neural Stem Cells | Proliferation of neural stem cells of 14-day-old rat embryo Over | |
| Primary | Neural Stem Cells | Differentiation of rat neural stem cells to neurons and glial cells | Over 7 days |
| Primary | Hippocampal Neuron | E18 rat hippocampal neurons, cultured in CO2 incubator for the first day | Over 3 days |
| Primary | Cardiac Myocite | Neonatal rat heart, fetal mouse, heart beat synchronization Over 3 | |








Simon Watkins and Claudette St. Croix Center for Biologic Imaging, University of Pittsburgh



Department of Genetic Engineering Kindai University




Tokyo Institute of Technology



Stage Top Incubator®






Features

Stress-Free Quality

Intuitive operation and varieties of new functions are included to support cell culturing without stress.

In addition to PID control, Continuous Current Control minimizes the focus drift generated by thermal expansion and it also prevents light intensity change compared to the conventional ON/OFF control.



- ■ Programmable Control

- STX-APP (Software)-----

Simple operation of GUI will assist to visualize the preparation to setting and lead your cell culture to success.



■ Screen Capture-----

Captures the PC screen to transfer images to smart-phones and tablets Enables to see the image at home.

* PC must be connected with internet



Data Logging --

Logs the temperature of each heaters, sample temperature and gas concentration and saves the data in

The system includes the software

concentration as this function allows

to expand the variety of experiments.

to program temp, and CO₂/O₂



TSU-200F

All in one package incubator

Including the following accessories as standard.

- SET model ------

· Temperature Controller



STXG

With built-in digital gas mixe **STXF** With built-in analog flow meter



WSKMX



· Extension Wire · Software STX-APP

· USB cable · Gas tube

Dish Attachments



ATX-W For well-plate For ATX-D, ATX-CSG For 35/50/60mm dish ATX-CSG For slide glass, chamber slide and chambered coverglass · Dish Fixing Lids

LX-W

For well-plate LX-D35 For 35mm dish LX-D56 For 50/60mm dish

LX-CSG For slide glass, chamber slide and chambered coverglass

■ Options -----

· Stage Adapter



with 160×110 (mm) opening

GSI2X-K For GSI2X For XY motorized stages · Dish Attachment



UNIV2-D35-2

UNIV2-D35-4



UNIV2-D35-3



UNIV2-D35-6

 \frak{X} The Dish Attachment for 35mm dish \frak{X} 5 is also available.


Line-up

WSKMX series

- Leica manual/motorized stage
- Sample temperature: 30 40°C



■ For well-plate and small vessels use









STXG-WSKMX-SET

STXF-WSKMX-SET

DMIWX series

- Leica manual/motorized stage (for Laser Safety Hood)
- Sample temperature: 30 40°C



■ For well-plate and small vessels use

100%CO2 gas cylinder use

Premixed gas cylinder use

STXG-DMIWX-SET STXF-DMIWX-SET

35 50 60 Chambered Chambered Chavenberg

GSI2X series

- For Leica SP8/SP5 Super Z Galvo stage For small vessels use
- Sample temperature: 30 40°C

100%CO2 gas cylinder use

Premixed gas cylinder use

STXG-GSI2X-SET STXF-GSI2X-SET

DLSX series

- For Leica SP8/SP5 Super Z Galvo stage
- Sample temperature: 30 40°C



100%CO2 gas cylinder use

■ For 35mm dish

Premixed gas cylinder use

STXG-DLSX STXF-DLSX

35_{dish}

WELSX series

- For manual/motorized/mechanical stages For small vessels use
- Sample temperature: 30 40°C ■ Chamber size is the same as wellplates



Model STXG-WELSX-SET 100%CO2 gas cylinder use

Model STXF-WELSX-SET Premixed gas cylinder use

Depending on the stage, a stage adapter might be required. Please contact Tokai Hit.





Cooling/Heating Chamber * Cooling/Heating Chamber is not compliance with CE

Sample temp.: 15 - 40°C (with dry lens) / 20 - 40°C (with oil/water immersion lens)



KRIX series

- For XY manual/motorized stage
- With Chiller Unit
- Sample Feedback regulation
- For small vessels use





100%CO2 gas cylinder use


Premixed gas cylinder use

Model STXGC-KRiX-SET Model STXFC-KRiX-SET

Uniform Temperature Distribution ------

Normally, it is difficult to control around room temp. because there is not big difference between room temp. and sample temp.. Since KRi series has both cooling and heating function independently, it can control around room temp. precisely

Heating (Sample: 37°C)



· Dish Attachments



Model KRiX-D35 Model ATX-D Model KRIX-CSG

Heating only (optional) Model ATX-CSG

Dish Fixing Lids

(Included to the system as standard) Model LX-D35

Included to the system as standard) Model LX-CSG

For upright microscopes

Sample temp.: 37°C

UKX series

- For XY mechanical stages of upright microscopes
- For small vessels use



Model STXG-UKX-SET 100%CO2 gas cylinder use

Model STXF-UKX-SET Premixed gas cylinder use

·■ Opening/Closing Top Heater -------Metal Top Heater with this function make it easy to set the object positioning before imaging.





· Dish Attachment

| For 35mm dish | UKX-D35 |
|------------------|---------|
| For 50/60mm dish | UKX-D56 |
| For slide glass | UKX-SG |

| Diacket | |
|-----------------------------------|-----------|
| For manual stage | UKX-STD |
| For Narishige fixed stage | UKX-FNS |
| For Prior Z-deck | UKX-ZD |
| For stages with 160×110mm opening | UKX-SPC-3 |

^{*} One-set is included as standard

· Lens Heater

| Lens Heater | UKX-LHD |
|-------------|---------|
| | 1.1 |

Lens Heater Options

| Lens Heater Adapter | UKX-LHA-□□ |
|---------------------|------------|
| Seal Ling | TMU-□□ |

^{*}One-set is included as standard

External Humidifier

Eliminates the need of refilling internal/external water for more than 3 - 4 days. By using this system with internal humidifier, it covers edge to edge of 96-well plate with stable and high humidity throughout the experiment.



SIMPLE add-on system for all Tokai Hit incubators

short to long-term imaging

STABLE cell culturing from

Model TPIDE-HUMID

Specifications

Temp. Controller

Temp. setting range: Ambient + 5°C - 60.0°C

Bottle capacity: 500ml

Heater dimensions: W100 × D110 × H110 (mm) Controller dimensions: W85 × D135 × H30 (mm) Components: Temp. Controller, Bottle Heater,

Water Bottle, Gas Tube set

Bottle Heater

Time Lapse movies 96-well plate Pictures are courtesy of N.Komatsu, A.Sakaue-Sawano and A.Miyawaki RIKEN Center for Brain Science, Saitama, Japan Cell cycle progression in Hela cells

(System image)



Enclosure for microscopes

ThermoBox

Maintains a stable cell culturing environment at places where the temperature fluctuation occur. By isolating the microscope from the envionment, it also prevents the focus drift caused by the thermal expansion of microscope itself.

Features

ThermoBox for DMi8



No duct required

Saves your working and setting space with built-in fan heaters. No air-ductis required for heating.

Anti-vibration heater

With anti-vibration design, the system can be used under confocal without image drift.

> Anti-vibration test movie



Available as a simple dark box

The black type has the property of light shielding and can be used as a simple dark box.


Front panel transparent model is also available as customization.

Specifications


- Dimensions of box: W715 × D440 × H400 (mm)
- Dimensions of controller: W95 × D305 × H211 (mm)
- Temp. setting range: Ambient 40°C (With heater)

Easy setup


Special tool is not required during installation and most of fixing is done by thumb screws.



<Side>



<Top>



Line-up

Live cell package

All the items are included for cell culture. ThermoBox Non-heater chamber CO₂ regulation **Dish Attachments** * Dish attachments for wellplate, 35mm, 50/60mm dish, slide glass, chamber slide and chambered cover glass are included.

| Microscope | Color type | CO2 gas cylinder | Model |
|------------|------------|------------------|---------------------|
| DMi8 | Black | 100%CO2 | Model DMi8TB-WSKM-G |
| DIVIIO | | Premixed | Model DMi8TB-WSKM-F |

^{*}Depending on the accessories (camera, stage etc.), the model may be a customized model. Please contact us for details.

ThermoBox only

| Microscope | Stage | Color type | Heater | Model |
|------------|---------------------------------|-------------|--------------------|-----------------------|
| | Motorized | D - | With heater | Model DMi8TB-BK |
| DMi8 | stage | Black | No heater | Model DMi8TB-BK-NH |
| DIVIIO | 3 plate stage (motorized) Black | With heater | Model DMi8TB-3E-BK | |
| | | RIACK | No heater | Model DMi8TB-3E-BK-NH |

^{*}Depending on the accessories (camera, stage etc.), the model may be a customized model. Please contact us for details.

Options

| Model DMi8TB-CLP | Replacable transparent front door |
|-------------------|--|
| Model TPIDE-HUMID | External humidifier system (refer to page 8) |

Add-on options

We offer the suitable solutions depending on your experiments.



Program fluidic control system

Perfusion, Media Exchange, Drug Delivery and Mixing can be easily programmed and done without disturbing your sample.

Model PMD-D35

%For STX/STR/INU Chamber ★For 35mm dish

System Image


[Specification]

Continuous Perfusion: 40 μ L/min - 100 μ L/min Media Exchange volume: 0.6ml - 5.0ml Media Exchange Number: Maximum 10 times

Drug Delivery: 20 μ L -

Controller size: W175 × D175 × H195 (mm)



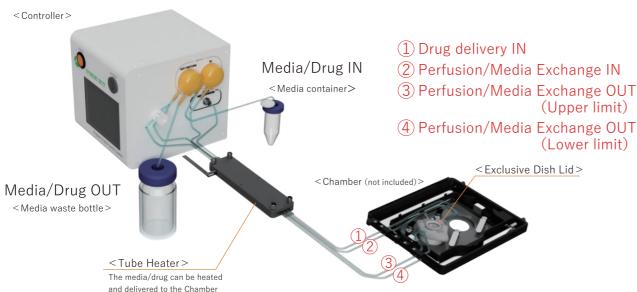

[Components]

- · Controller
- Tube Heater
- · Tubes (IN/OUT, with drug delivery fitting)
- · Media containers (For perfusion, Media Exchange)
- · Multi Fluidic Lid (PMD-D35FME) for 35mm dish
- · Diamond Insert (KS-DIA) for 35mm dish (100 ul media exchange)

*Media waste bottle is not included

- Enables to mix the media and drug to be uniformly after the drug delivery.
- Setting of suction / supply liquid volume at a finer flow rate is possible.
- Regulates the system with TTL IN/OUT.
- High-repeatability experiments are possible by keeping the media level evenly.
- With a built-in tube heater, one fluidic control system can be completed with one system.
- Supports general 35mm dish.
- Manages each user's program individually by using USB memory.

Perfusion/Media exchange system

Perfusion/Media exchange without removing a dish lid is possible. Prevents media evaporation and contamination during long-term imaging.



One-push drug delivery system

Rapid and vibration-free drug delivery is possible. Prevents media evaporation and contamination during long-term imaging.


Model KSX-Type2 *For STX/STR Chamber KS-Type2 *For INU Chamber

Dosage : 20 *µ* ℓ - 100 *µ* ℓ

(Contact us if different dosage needed) Controller dimensions: W100 × D165 × H116 (mm)

Silicon tube: OD 3.0mm, ID 1.0mm

(Tube of the Dish side is disposable)

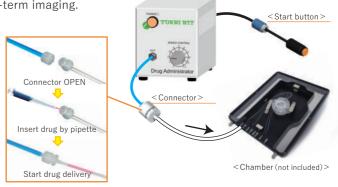

for Living cells for your imaging ®

Digital Gas Mixer

Digital Gas Mixer for Stage Top Incubator. You can choose depending on the usage gas cylinder.

For STX series



Model STX-CO2O2

For low oxygen (Hypoxia)

O2 concentration : 0.1 - 18.0% CO₂ concentration: 5.0 - 20.0% Gas cylinder: 100%CO2 & 100%N2 Dimensions: W160 × D271 × H250 (mm)



Model STX-CO2

For CO₂ concentration CO₂ concentration: 5.0 - 20.0% Gas cylinder: 100%CO2

Dimensions: W115 × D271 × H250 (mm * For STXF Controller

Model STX-O2

For O₂ concentration

O2 concentration: 0.1 - 18.0% Gas cylinder: 100%N2 Dimensions: W115 × D271 × H250 (mm)

* Must use with STX-CO2

Stand alone



Model **GM-8000**

For low oxygen (Hypoxia)

O2 concentration : 0.1 - 18.0% CO₂ concentration: 5.0 - 20.0% Gas cylinder: 100%CO2 & 100%N2 Dimensions: W160 × D260 × H187 (mm)



Model **GM-3000**

CO₂ concentration & flow rate

CO2 concentration: 1.0 - 20.0% Flow rate : 50 - 200 ml/min Gas cylinder: 100%CO2

Dimensions: W121 × D174 × H157 (mm)

Mini CO2 regulator * MG1 is only available in the US and Japan at this moment.

There is no need to prepare a large gas cylinder and no regulator operation is required. The gas is supplied at the optimal flow rate for the Tokai Hit incubator with one push.

Model MG1

[Specification]

Output gas pressure: 0.1 MPa Usable time: about 3 days / 1 cartridge Dimensions: W135 x D182 x H237 (mm) Weight: 2.5 kg

■ Consumable gas cartridge

Consumable gas cartridge is available.

Please contact LELAND with the part number: 88100Z.

- Cartridge size: 74 g

- Thread design: 5/8 - 18UNF





Add-on options

We offer the suitable solutions depending on your experiments.



Reusable 35mm dish *Cyto-cell Chamber (Auto-clavable)

< Collaborative development with Prof. Takafumi Inoue, Waseda Univ. >

For a small amount of medium



Model SCC12-D35-SET Cover glass size : ϕ 12.0 mm Observation area : ϕ 9.6 mm

For wide range observation



Model SCC25-D35-SET

Cover glass size : ϕ 25.0 mm Observation area : ϕ 21.0 mm

[Features]

- 1. Whole bottom observation is possible. No interferes with an objective even under high magnification
- 2. Running costs can be reduced. By changing the consumable parts, the dish can be reused repeatedly.
- 3. Observe with small amount of media.

«Consumable parts (Stainless steel plate, cover glass etc.) are also available

[Assembly]






























Department of Life Science and Medical Bioscience Faculty of Science and Engineering, Waseda University

Digital Thermometer for research



Precise temperature measurement is possible by using a thin sensor with Teflon covering and excellent chemical resistance.

MC1000

Indicate temp. by 1°C or 0.1°C K-type thermocouple

< Components > Digital Thermomete

Thermo Probe (TSU-200F)

For media exchange and drug delivery with incubation system for upright microscopes etc..



■ Extension Wire (1.5m)

■ Thermo Prove (Sensor type) Model **TSU-200F** Model HD1500

IN/OUT Pipe for Media Exchange/Drug Delivery



PSBD1 Pipe OD 1.1mm

PSBD1H Pipe OD 1.1mm (with side holes)

PSBD2 Pipe OD 2.1mm

PSBD2H Pipe OD 2.1mm (with side holes)

35mm Dish Spacer

When using the 35mm dish from IWAKI, Greiner and Nunc, recommended to use Dish Spacer at the bottom of the dish.




Model 35DI-BS For 35mm dish from IWAKI



Model 35DGN-BS

For 35mm dish from Greiner and Nunc




The Institute of Scientific and Industrial Research, Osaka University

Customization

We have experience

More than 100 customized products per year.



Hearing





We are accepting customization according to the application and conditions. Please feel free to contact us.





Assembly


Customization reference

Incubation system for MED64

This device has been designed on the assumptions of an experiment of electro physiology. Enable the low noise attribution under the cell culturing environment.

| With built-in digital gas mixer | Model INUG2M-MED |
|---------------------------------|-------------------|
| With built-in analog flow meter | Model INUM-MED-F1 |
| Temperature Controller only | Model INUM-MED |







KW / KD series

BOX-type ThermoPlate with a gas port.

- · For inverted microscope
- · Setting temp.: Ambient~50°C (Plate temp.)
- · Top Glass Heater prevents the condensation of the dish.
- · Double Heater system (Top Heater/Stage Heater) keeps the suitable sample temp.

| For well-plate use | Model TPiD-KW |
|--------------------|---------------|
| For 35mm dish use | Model TPiD-KD |



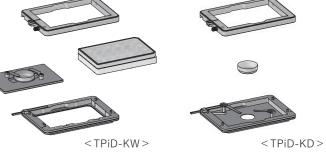

Integration/Customization

We support and design the instruments for customer's requirement with over 20 years technology and knowledge. Please let us know your needs and requirements. We can designed customized system for you. We are flexible to design different size, temperature regulation, setting range, etc.

e.g. looking for a system for Patch clamp, system integration, unique design/size to installing to your system, etc.


We value your needs and requirements. If you have any questions or concerns, please feel free to contact us.

Glass/Metal Heater for microscope ThermoPlate®

Persues high-end "User-Friendliness"

Ensure more accurate and more reliable thermal control of the specimens during the observation under a microscope. Wide product range supports Biotechnology Science and Industry.







More downsizing and weight saving of cotroller compared to TP/TPX series.

Multi-function system supports temperature management in various fields such as biological science.

Features

Compact Controller

Miniaturizes the controller to be as small as a smart-phone It is very useful for space saving in the clean bench.

Controller dimensions : W85 \times D135 \times H30 (mm)

Size: 232 (cm³) <u>*82% decreased</u>
Weight: 170 (g) *62% decreased

In addition to flat placement (left), stand upright (center) and wall hanging (right) are available with attached mounting hook depending on the location of use. The mounting hook is thin but durable design with a load capacity of 2 kg.

< Flat placement >







Thermo Plate

TOKRI HIT


Simple temp. measurement


Attached sterilized sensor can measure the actual temperature and correct the plate suface temperature. Enable to monitor and log the data of temperature which the sensor measures.



Continuous Current Control

In addition to PID control, Continuous Current Control minimizes the focus drift generated by thermal expansion and it also prevents light intensity change compared to the conventional ON/OFF control.





10 year free-repair service for glass breakage

Applied strengthen glass or hard glass for the glass heater and with 10 year free-repair service for glass breakage. No more glass breakage and no more stopping your experiment.

*1. Depending on the model





One-touch calibration

Easy calibration to set the suitable PID value on your usage environment is available with just one-touch.

* Tokai Hit's ThermoPlate is calibrated with the controller and the plate as a set to make the center of the plate temp. to be at 37.0°C when the room temp. is 25°C prior to the shipping.

Plate LED Indicator

Plate LED Indicator visualizes the plate condition without looking at the controller.

Green LED lights up when the glass heater is ready.



| Statement of LED | Condition of the plate |
|------------------------------------|---|
| Lights up | The plate surface temp. is stable at the setting temp |
| Blinks slowly (1.0 sec. period) | Running Calibration. |
| Blinks fast (0.2 sec. period) | An error occurred. |

* Plate LED is attached to some major models.





Reference movie: ICSI



Glass Heater Line-up

Tokai Hit's Glass Heaters

Temp. setting range: Ambient - 60°C (* Depenging on the model)

Original clear glass heater maintains stable temperature.

Supports the needs in different various fields such as Time-Lapse in low magnification and/or IVF field.



plicable stage : XY manual/motorized stage with 160 imes 110 mm opening



Model TPi-SQFTLX (1991)

Glass thickness: 0.5 (mm)

Plate dimensions: W160 × D110 (mm) Heating area: W135 × D95 (mm)



Microscope: DMI6000B/4000B/3000B

plicable stage: XY manual/motorized stage with 160×110 mm opening



Model TPi-SQX (19) Glass thickness: 0.5 (mm)

Plate dimensions: W160 × D110 (mm) Heating area: W128 × D84 (mm)



Microscope: DMi8, DMI6000B/4000B/3000B

pplicable stage: Slim stage with 88 mm round opening



Model TPi-RSRX (1997)

Plate dimension : φ 88 (mm)



nverted

Microscope: DMi8, DMI6000B/4000B/3000B

pplicable stage : Mechanical stage

roscope : DMIRB



Model TPi-SQMX (1997) Glass thickness: 0.5 (mm)

Plate dimensions: W165 × D105 (mm) Heating area: W129 × D86 (mm)





Model TPi-GSIGX (1991)

Glass thickness: 0.5 (mm) Plate dimensions: W129 × D87 (mm) Heating area: W111 × D62 (mm)



pplicable stage: XY manual stage with 150×150 mm opening




Model TPi-RSLTX (19) Glass thickness: 0.5 (mm)

Plate dimensions: W150 × D150 (mm) Heating area: W130 × D130 (mm)

For upright microscopes

olicable stage: XY mechanical stage



Model TPi-SX (19) Glass thickness: 0.5 (mm)

Plate dimensions: W142 × D115 (mm) Heating area: W128 × D95 (mm)



For stereo microscopes

ion base: Transmitted Light Base TL RCI/RC etc.



Model TPi-TLBaseX (1991)

Glass thickness: 1.0 (mm)



Plate dimensions: W219.5 × D169.5 (mm) Heating area: W190 × D134 (mm)

UNIVERSAL

or various types of illumination bases



Model TPi-UNIX (19)

Glass thickness: 1.5 (mm)

Plate dimensions: W435 × D220 (mm) Heating area: W400 × D175 (mm)

Leg adjustment: 75 - 100 (mm) * Temp. setting: Ambient - 50°C



With 10 year free-repair service for glass breakage.



With Plate LED Indicator.



Stereo

Large Glass Type

For various types of illumination bases



Model **TPi-W**

Glass thickness: 1.5 (mm)

Plate dimensions: W230 × D180 (mm)

Heating area: W180 × D140 (mm)

Model TPi-WL

Glass thickness: 1.5 (mm)

Plate dimensions: W310 × D220 (mm) Heating area: W250 × D170 (mm)

Metal Heater Line-up

For oil/water immersion objective and high-magnification objective imaging

Temp. setting range: Ambient - 60°C

Focus drift is caused by thermal expansion from the ordinary ON/OFF regulation.

Tokai Hit is applying Continuous Current Control regulation as standard to minimize focus drift.



Microscope: DMi8

plicable stage: XY manual/motorized stage with 160×110 mm opening



Model TPi-SQH26FT

Plate dimensions: W160 × D110 (mm) With a hole (ϕ 26 mm)

* Surface flat type


pplicable stage: XY manual/motorized stage with 160×110 mm opening

Plate dimensions: W160 × D110 (mm)

Model TPi-SQH26

With a hole (ϕ 26 mm)

Microscope: DMI6000B/4000B/3000B



Model TPiD-I2X 199



Plate dimensions: W160 × D110 (mm) *2 in 1 type

Glass: W68 × D95 (mm)

Metal: With a hole (φ 25 mm)





Model TPi-GSIH26

Plate dimensions: W129 × D87 (mm) With a hole (ϕ 26 mm)

Options




Lens Heater Model TPIE-LH

Temp. setting range: Ambient - 45°C Prevents heat loss from the sample especially when using oil/water immersion objective and high-magnification objective.



Tube Heater Model TPIE-TH

Temp. setting range: Ambient - 50°C A compact barrel-type heater. Simply wrap the media tubing for heating the media before inserting it to Chamber Unit.



Hot Plate

Model TPIE-SP/SPE

Temp. setting range: Ambient - 45°C Light-weight and thin aluminum thermal plate. TPiE-SP : W482 × D282 (mm) TPiE-SPE: W282 × D232 (mm)





Reference movie: ICSI

2-channel controller (Option)



2 plates can be controlled by TPiD controller. Every combination is possible.



Entire Surface Heating Plate

Temp. control before/after observation

Temp. setting range: Ambient - 50°C

Since the entire surface of the plate is heated, it can manage the temp. of the sample under observation as well as the sample before/after observation. It is very useful when dealing with many samples.

For stereo microscopes

Illumination base: Transmitted light base TL RCI/RC etc.

Model TPID-TLDX (19)

Glass thickness: 0.5 (mm) Plate dimensions: W380 × D206 (mm) Heating area: < Glass part > W128 × D95 (mm)



Enables to keep the vessels warm before and after observation.



ThermoPlate for Vitrification warming

For thawing process of frozen embryo

Temp. setting range: Ambient - 60°C





Base dimensions: W435 × D280 (mm) Plate dimensions: W230 × D148 (mm) Heating area: W95 × D128 (mm) × 2

Glass thickness: 0.5 (mm) Leg adjustment: 75 - 100 (mm)

Cooling/Heating Plate * Cooling/Heating Plate is not compliance with CE

Best for observing yeast, plants, marine samples, cultured cell, C. elegans and/or Planarian, etc.

Temp. setting range (Plate surface): 4 - 60°C

With electronic cooling element (Peltier module) and original control system, it allows responsive cooling and heating regulation.

* The plate may build the condensation at the bottom when the setting value (SV) of the controller set below 15.0°C (depending on the lab temperature). The system may not be suitable for

- Long-term imaging

- Rooms with high humidity

37°C Cultured Cell 28°C Zebrafish 25°C Drosophila 20°C C. elegans

Usually, it is difficult to control the temperature around room temperature because of the small temperature difference between the room temperature and the sample temperature. However, Tokai Hit Cooling/Heating Plate has both cooling and heating functions and can control the temperature around the room temperature accurately without any change-over switch.

It also can be used for controlling activation of the common samples which normally cultured at 37.0 degree C by lowering the temperature or observe expressions of samples at each temperature.

Microscope: DMi8, DMI6000B/4000B/3000B

cable stage: XY manual/motorized stage with 160×110 mm opening

<With Chiller Unit>

Model TP-CHSQ-C

Plate dimensions: W160 × D110 (mm) With a hole (ϕ 20mm)

plicable stage: Mechanical stage

Microscope: DMi8, DMI6000B/4000B/3000B

< With Chiller Unit > Model TP-CHSQM-C

Plate dimensions: W165 × D105 (mm) With a hole (ϕ 20mm)

DMi8. DMI6000B/4000B/3000B

cable stage: Slim stage with 88 mm round opening

< With Chiller Unit >

Model TP-CHSL-C

Plate dimensions : φ 88 (mm) With a hole (ϕ 20mm)




Microscope: For upright microscopes ble stage: XY mechanical stage

< With Chiller Unit>

Model TP-CHS-C

Plate dimensions: W110 × D110 (mm) With a hole (ϕ 20mm)

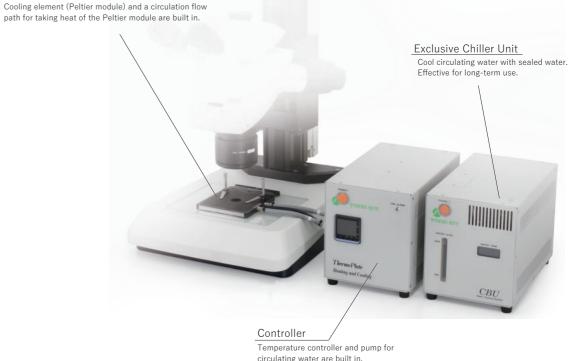

circulating water are built in.